

HIGH-PERFORMANCE LIQUID CHROMATOGRAPHY



New Modules

New Accessories

New Improvements

Chromaster

Outstanding performance


Easy-to-use

Robust



HPLC for today and tomorrow

MS Detector is also available

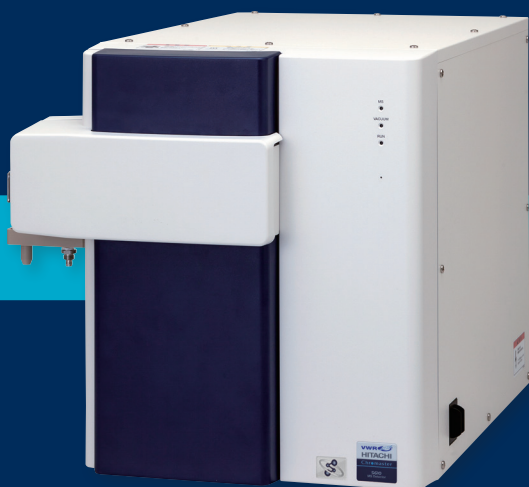

EASY – ACCURATE – COMPACT

Hitachi offers a new MS detector, designed for HPLC users, that is different from existing mass spectrometers.

Outstanding performance

Excellent reproducibility given by a highly stable and robust system.

Pump

Improved gradient performance and the excellent flow rate precision

The Chromaster has a new low-pressure mode called High Frequency Mode (HFM), which utilizes a double switching function of proportioning valves. HFM and the Hitachi high speed realtime feedback control system, greatly suppress liquid pulsation for improved reproducibility of gradient and retention times.

Autosampler

Excellent injection volume precision and low carry-over

The newly adopted high-precision syringe drive unit provides excellent injection volume precision. Hitachi has eliminated the dead volume in the autosampler by adopting a new syringe and a new syringe pumping method that washes the needle outer wall. The result is an accurate autosampler with extremely low carry-over.

Column Oven (5310 Column Oven)

Pre-heating function and a wide temperature control range

The block-type pre-heating function based on Peltier heating and cooling control delivers excellent symmetric and sharp peak shape. The oven can regulate^{*1} temperature from 15 degree below ambient to 125 degree above ambient. The oven can accommodate various columns.

*1 Temperature setting range: 1 to 85°C

Diode Array Detector

Excellent qualitative analysis performance, and extremely low noise and drift

With a wide wavelength range (190 nm to 900 nm) and excellent resolution (1,024-bit diode array), the Chromaster Diode array detector delivers excellent high-resolution analyses. With a noise level comparable to a UV detector, the Diode array detector is capable of supporting high-sensitivity analyses.

The adoption of a variable air-volume fan and the provision of a specially designed cover on the spectrometer minimize light leakage and achieves a further reduction in drift. A variable air-volume fan for the diode array detector and a new cover designed for the spectrometer greatly reduce the temperature change in the detector module.

UV and UV-VIS Detectors

Two-wavelength, simultaneous high-sensitivity detection of drug impurities

The two-wavelength detection function permits measurements at short data acquisition interval of 400 ms^{*2} and 800 ms per wavelength, resulting in chromatograms with high resolution.

*2 The 400 ms interval is available only if the wavelength delta is 160 nm or less.

Thermostat flow cell

The thermostat^{*3} flow cell maintains a constant ambient temperature changes. As a result, the detector baseline is steady and data reliability is improved.

*3 Optional

Easy-to-use with excellent reproducibility

Beyond the simplicity of operation and ease of use, a critical requirement

is to have a system that is easy to use and provides excellent reproducibility.

GUI controller

Provides an attractive user interface and permits the operation of modules on a stand-alone basis.

The GUI controller^{*4} comprises a color LCD monitor and a touch-panel system for ease of operation. (Some modules are not compatible.)

*4 Optional

Auto-purge function

Startup tasks of pump, simplified

From Chromatography Data Station^{*5}, you can set any UI Co

to be purged automatically. (Pumps with or without auto-purge valve are available.)

*5 See p. 22.

Auto-plunger washing function

Prevents the precipitation of salts onto the plunger surface.

As a standard, Chromaster includes a washing mechanism that prevents damage to the pump seal or the plunger by salt precipitation from the mobile phase. A combination of Plunger Washing Pump^{*6} and CDS permits automatic washing after each analysis run.

*6 Optional

Low-volume degassing unit

Shorter solvent purging time

Over 50% shorter purging time compared to conventional degassing units.

The degassing unit has a 6-channel autosampler, and reduces the amount of solvent used. The degassing unit has a 6-channel

Autosampler with thermostat (5260 Autosampler)

Capable of heating up to 45 °C

The Autosampler with thermostat is capable of controlling the temperature (in a vial) ^{*7}. This level of vial temperature control broadens the application range and maintains sample stability by preventing crystallization of sample components in the vial. (Autosamplers are available with and without a thermostat.)

*7 Optional

Dedicated degassing unit for autosampler (5260 Autosampler)

Space-saving built-in degassing unit

The Chromaster autosampler incorporates a dedicated degassing unit^{*8}. When the user wants to operate the Chromaster autosampler without Chromaster pump, this degassing unit has great utility. Moreover, because it can be a built-in unit, the degassing unit does not take up extra bench space.

*8 Optional





A specially designed cover for the spectrometer and a variable air-volume fan

Reduced lamp stabilization time (Diode array detector)

A variable air-volume fan for the diode array detector and a new cover designed for the spectrometer greatly reduce the temperature change in the detector module. The result is a 30% reduction^{*9} in lamp stabilization time.

^{*9} in-house comparison

Column oven (5310 Column Oven)

Easily accommodates a 300 mm analytical guard-column

The door, which opens in an L-shape pattern and with internal dimensions 375 mm wide and 114 mm high, facilitates the connection and stowing tasks for a guard-column and column. The oven can accommodate up to three 300 mm columns.

Column management system

Column log information is saved in the ID tag

The Chromaster column management system^{*10} manages the Log information on analytical columns and guard-columns from any manufacturer. Log information can be written and read through a connector or a PC USB port mounted on the column oven. ID Tags can be used repeatedly.

^{*10} Optional

Solvent cabinet with a power supply box

A large space for a number of bottles in one place.

The following solvent bottles can be mounted on the organizer (a solvent cabinet with a power supply box):

Example

3,785 l (U.S. gallon bottle) × 2 + 500 ml × 2

3,0 l (Japanese gallon bottle) × 2 + 500 ml × 2

2,5 l (EU gallon bottle) × 2 + 500 ml × 3

1,0 l bottle × 5 + 500 ml × 2

System size

Reduced height and minimized footprint

Most optional accessories are internally mounted to reduce HPLC system height. At the same time, the handle located on the front side of the organizer moves vertically for easy access to solvent bottles. With a module width of 340 mm^{*11} and a depth of 440 mm, the system provides space savings.

^{*11} Exclusive of the column oven

Robust

The Hitachi reputation for instrument robustness and reliability continues with the Chromaster, which is made using stronger materials and is manufactured according to Hitachi's strict quality control standards.



Designed for longevity

The external covers are made of heat-resistant, chemical-tolerant, and UV irradiation-withstanding materials. The internal walls of the module are made with stainless steel for the prevention of corrosion owing to humidity and any adverse effect on the module in the event of solvent

Other functions

- The autosampler has a door lock mechanism for safety (5260 Autosampler).
- During the lamp replacement operation, power is automatically shut off.
- A leak sensor is installed in all modules.
- To guard against any leakage of non-volatile solvents in the column oven, the column oven incorporates a solvent leak sensor and a gas sensor.

Introducing the Chromaster[®] modules

F u l l i n g t h e u s e r '

Data reliability

Intuitive operation based on an LCD touch panel

Attention to details

Ease of maintenance



ORGANIZER p 18

DETECTOR p 14

CONTROLLER p 19

COLUMN OVEN p 12

AUTOSAMPLER p 10

PUMP p 9



UHPLC entry-level model with a wide application range for HPLC users

compatible not only with conventional 40 MPa system but also with 60 MPa system. The 60 MPa system, which can be used with columns containing 2,0 µm or smaller particles, and core-shell columns, is capable of conventional HPLC analyses and also ensures improved resolution performance and shorter analysis time.

Analysis Example from the Chromaster 60 MPa System

By connecting the Chromaster 60 MPa system to a UHPLC column, high-speed high-resolution analysis can be performed. The 60 MPa system can also be used as an entry-level model for UHPLC.

Conditions

Sample: Alkylphenones

Column: LC101 (4.6 mm ID, 150 mm L) × 1.5 µm

Column: Lachrom CR101 (4.6 mm ID, 150 mm L) × 2.0 µm

Column temperature: 40 °C

Mobility: AcH₂O, CH₃CN

Gradient mode: High Frequency Mode


Wavelength: 214 nm

The following options are used with UHPLC column

- Low dispersion piping kit
- Semi-mini (2.0 µm)
- Semi-fraction collector

HPLC column

4,6 mm ID, 150 mm L (1.5 µm)

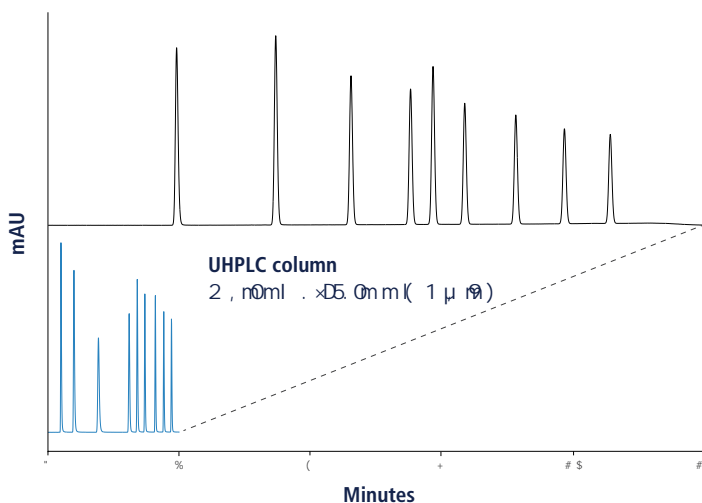

For users of UHPLC columns

To maximize resolution, a UHPLC column with 2.0 µm or smaller particles should be used. For the best resolution performance, diffusion contributions from components outside the column should be minimized. The following options are available as optional items.



Chromaster

Improved gradient performance and excellent flow rate precision

5110/5160 Pump

Excellent solvent delivery performance

One of the most important performance measures for HPLC is retention time reproducibility.

Excellent gradient performance resulting from the highly accurate solvent delivery by the

High Frequency Mode (HFM) of the proportioning valve make the high retention time reproducibility possible.

Analysis of alkylphenones 9 components

Gradient method (gradient-free) (H)F (Mixer - less)

Conditions

Sample: Alkylphenones

Column: Hitachi LaChrom C18

4 mm ID x 150 mm (µm)

Column temperature: 40 °C

Mobile Phase: A H₂O + 0,1 % TFA

B CH₃CN + 0,1 % TFA

Gradient mode: High Frequent Mode

Gradient time: 5: (305) > 5: (355)

— 5: (320, 1)


— 5: (350)

Injection volume: (100 µl)

Flow rate: 1 ml/min

Detection: 24 nm

Peak No.	Component	Retention Time	
		AVE	% R S D
1	Acetanilide	3,220	0,03
2	Acetophenone	5,397	0,04
3	Propiophenone	7,328	0,03
4	Butyrophenone	9,006	0,02
5	Benzophenone	9,593	0,02
6	Valerophenone	10,642	0,02
7	Hexanophenone	12,214	0,02
8	Heptanophenone	13,679	0,02
9	Octanophenone	15,026	0,02

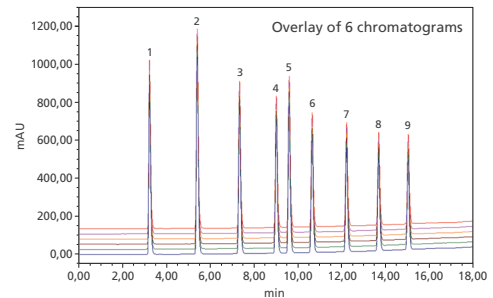


Pump options

6-channel degassing unit (optional)

- Solvent up to maximum flow rate autosampler

Auto-purge valve (Pump solvent to purge available)

- Flow rate: 0.1 ml/min (0.1 ml/min)
- This is the maximum flow rate

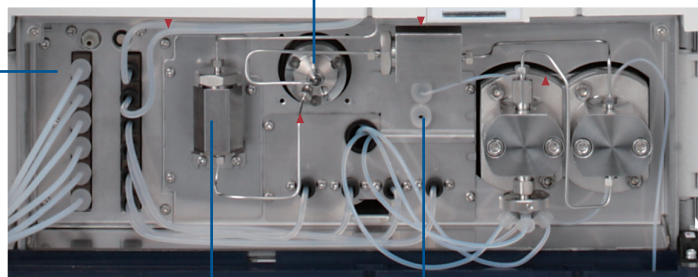

Conventional mixer

(Access to flow - pressure reduction)

(Can also accept semi-micro/dynamic mixers)

(Can install either of one from three mixers)

Plunger washing pump (optional)

- Flow rate: (mixed)
- This is the maximum flow rate
- Automatic plunger washing function per one analysis available with CDS

Notes

- (1) Plunger washing mechanism: standard
- (2) Automatic plunger washing using only Item (1) is subject to the following limitations:
 - Requires 5260 Autosampler
 - Not compatible with two-solvent washing for the needle inner

Two types of autosamplers are available to meet customers' needs

5260/5280 Autosampler



5260

Product lineup to accommodate various applications

To accommodate various HPLC applications, the Chromaster product lineup includes autosamplers with loop injection and direct injection.

As both autosamplers have a pressure range of 60 MPa, they are applicable to high-resolution, high-speed analyses of UHPLC columns as well as traditional HPLC.

Item	5 2 6 0	5 2 8 0
Sample injection system	Loop injection method	Direct injection method
Withstand pressure	60 MPa	60 MPa
Washing function	Equipped with built-in washing pump Two-solvent washing function	Wash solvent delivery by a syringe
Sample rack temperature control (Temperature setting range)	1 to 45 °C Capable of cooling and heating	1 to 35 °C cooling only
Sample capacity	Standard 120 × 1,5 ml Optional 72 × 4 ml	200 × 1,5 ml 128 × 4 ml


Excellent injection volume reproducibility supporting reliable analysis

The syringe and syringe moving part are optimized for each of the loop injection and direct injection systems. As a result, the measurement accuracy by the syringe is improved, resulting in excellent injection volume reproducibility.

Example: Injection volume reproducibility data

Conditions

Sample: 60 ppm Methylparaben
(Methyl 4-hydroxybenzoate)
Flow rate: 1 ml/min
Wavelength: 265 nm
Injection: 20 µl injection loop

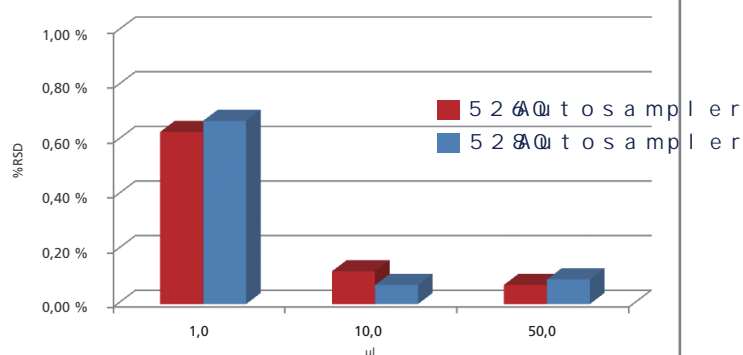

Low carry-over
≤0.003%
(under a specified condition)

Extremely low carry-over

To reduce the amount of carry-over, an autosampler must be engineered to eliminate the

The Chromaster autosampler, thanks to the design of the tube connections and injection port shape, ensures extremely low carry-over for both the loop injection system and direct injection system.




Chromaster



5280


Loop injection autosampler for lower carry-over

for the needle outer wall in order to achieve lower carry-over. As a result, the carry-over is as low as that from the direct injection system. In addition, the standard installation includes a two-solvent washing function for the needle inner wall to ensure low carry-over even for the analysis of the most persistent components.

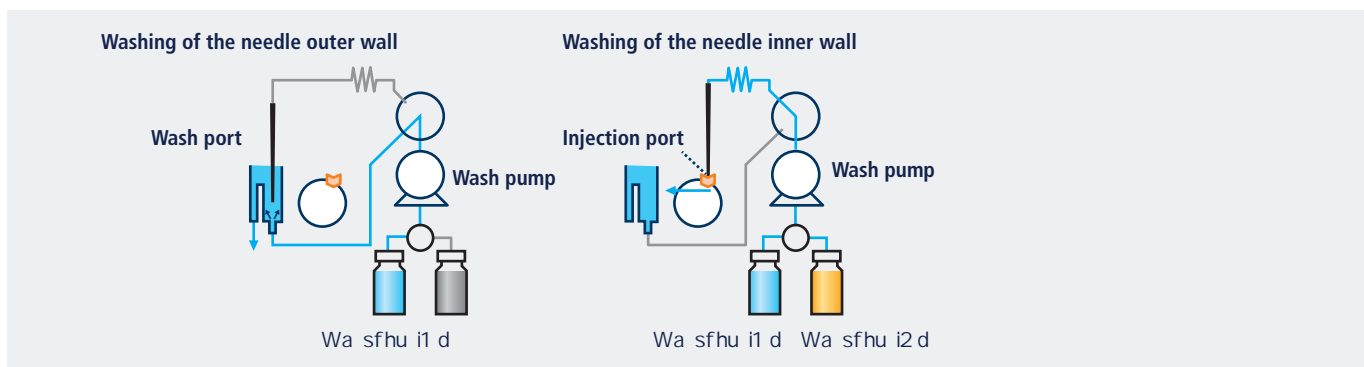

Additional settings to reduce carry-over

- Needle outer wall washing prior to sample drawing

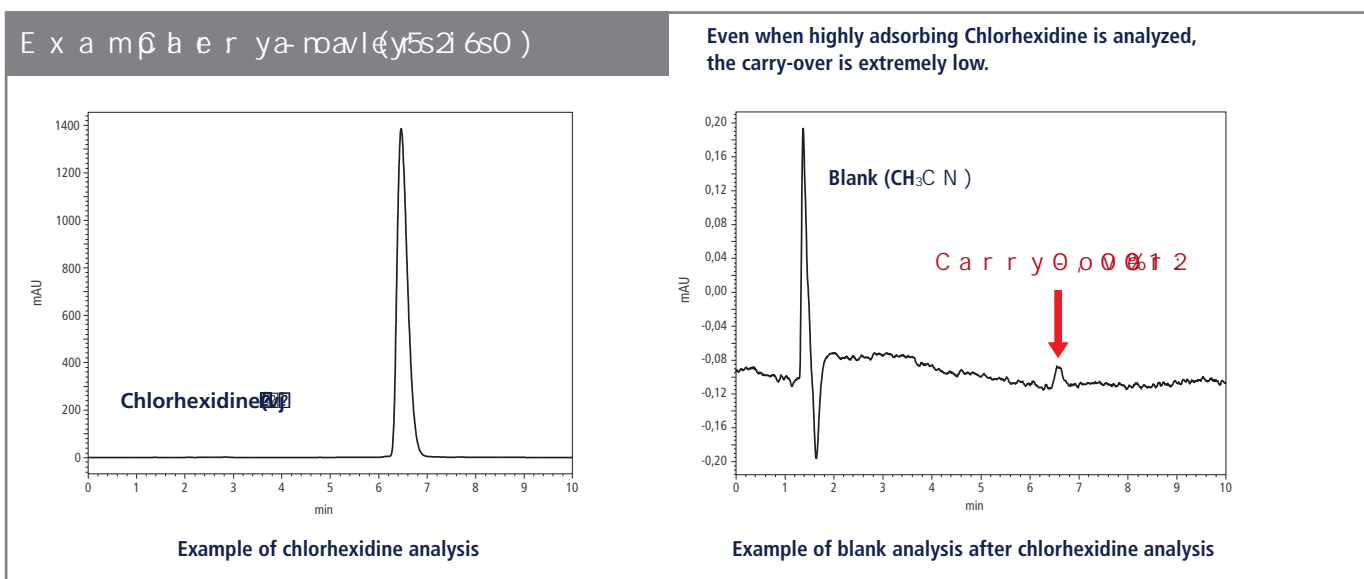

Generous size column compartment width of 375 mm

5310 Column Oven



The photo is a column oven with a GUI controller (optional).

Easily accommodates a 300 mm ana with a guard-column

The door, which opens in an L-shape pattern and with internal dimensions 375 mm wide and 114 mm high, facilitates the connection and stowing tasks for guard-column equipped column. The oven can accommodate up to three 300 mm columns.

Pre-heating function and wide temperature control range

The block-type pre-heating function based on Peltier heating and cooling control, delivers excellent peak symmetry and shape.^{*1}

Also, the oven has the capability to regulate^{*2} temperature from 15 degree below ambient

to 200°C (392°F) with 0.1°C (0.2°F) resolution.

Temperature range: 15°C (59°F) to 200°C (392°F)

Resolution: 0.1°C (0.2°F)

Pre-heating units



The photo represents a unit in which a part of the pre-heating cover is removed.




Column management system (5310 optional)

Hitachi column management system can manage the Log information on analytical columns and guard-columns from any manufacturer.

Log information can be written and read through a connector mounted on the column oven or USB port in the computer.

ID Tags can be used repeatedly.^{*3}

*1: Hitachi, Ltd. (2015)

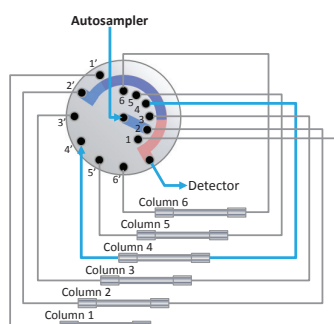

Valve option for method development (6310 optional)

6-column selector valve for method evaluation is also available.



Chromaster

Improved operability over a wider temperature range

6310 Column Oven



Temperature range of 4 to 90 °C*4 and superior temperature stability

- Faster heating and cooling time
- Temperature control range: [ambient temperature - 20 °C to 90 °C] temperature setting range
- Maximum column capacity of 6 x 100 mm columns or 300 mm x 3*5

*4: The range of temperature control depends on the ambient temperature.

Low volume pre-heating to suppress peak diffusion

The newly designed low volume pre-heating tube minimizes the peak diffusion while the temperature stability is maintained, resulting in high resolution analyses and high reproducibility.



A view of column oven accommodating columns

	5310	6310
pre-heat piping volume	39 µl	1 µl

Built-in 3-liter Waste Tank

A 3-liter Waste Tank is housed below the column oven. Typically, a waste solution container is placed underfoot, but now the space for the container can be utilized for other purposes, and safety is also improved.



3-liter Waste Tank

MEM column (6310 optional) g

MEM column (6310 optional) g

- A built-in spring presses the connection tube to the column inlet port, so the dead volume is kept
- pressure tolerance (Pressure resistance when used separately: 140 MPa) can be maintained even after repeated use.



MEM column fitting



5430 Diode Array Detector

Excellent qualitative analysis performance


With a wide wavelength range of 190 nm to 900 nm, the 1,024-bit diode array in Chromaster

Achievement of further low noise and low drift


The 5430 diode array detector is comparable to conventional Ultraviolet (UV) detectors for baseline noise to $0,5 \times 10^{-5}$ AU^{*1} (or less), and is capable of high-sensitivity detection. The adoption of a variable air-volume fan and the provision of a specially designed cover on

the detector (or less) and a reduction in lamp stabilization time by about 30% (In-house comparison).

Comparison of Diode Array Detector and UV Detector

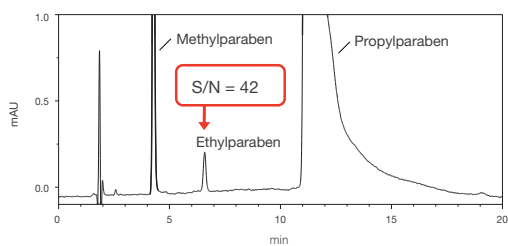


5 4 3 0 Diode Array Detector

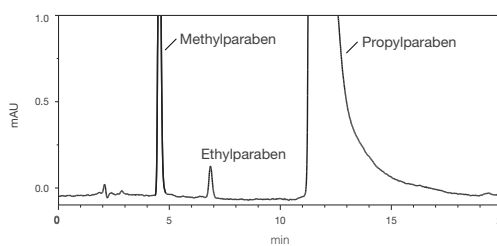

5 4 1 0 UV Detector

The noise level of the 5430 diode array detector is lower than that of the UV detector, which is highly sensitive.

Common features (5410/5420/5430)



The most accurate flow Ultraviolet (UV) region wavelength check by means of a built-in

temperature changes.

As a result, the baseline of detector is steady and data reliability improved.

The emission lines of built-in D2 and Hg lamps allow wavelength checks over the ultraviolet to visible range. As there is no physical change with the Hg lamp over time, the accuracy check will result in highly reliable data.



Chromaster

Excellent qualitative and quantitative analysis performance

5430 Diode Array Detector 5410 UV/5420 UV-VIS Detector



5410 UV/5420 UV-VIS Detector

Low noise, low drift, and a high sensitivity detection

A noise level can achieve $0,5 \times 10^{-5}$ AU^{*2} (or less) can be achieved, allowing better sensitivity than ever.

011V1P8037D1R700R700D
0E0281020VPE0181V3?
09200022(10)091V109

^{*3} (or less), these detectors deliver excellent


Two-wavelength simultaneous measurement function

The two-wavelength detection function^{*4} permits measurements at short data acquisition intervals of 400 ms^{*5} and 800 ms per wavelength. The result is chromatograms with sharp peak shapes.

^{*4} Controlled by CDS only

^{*5} 400 ms is available only if the wavelength interval is 160 nm or less.

Example: Two-wavelength simultaneous analysis data

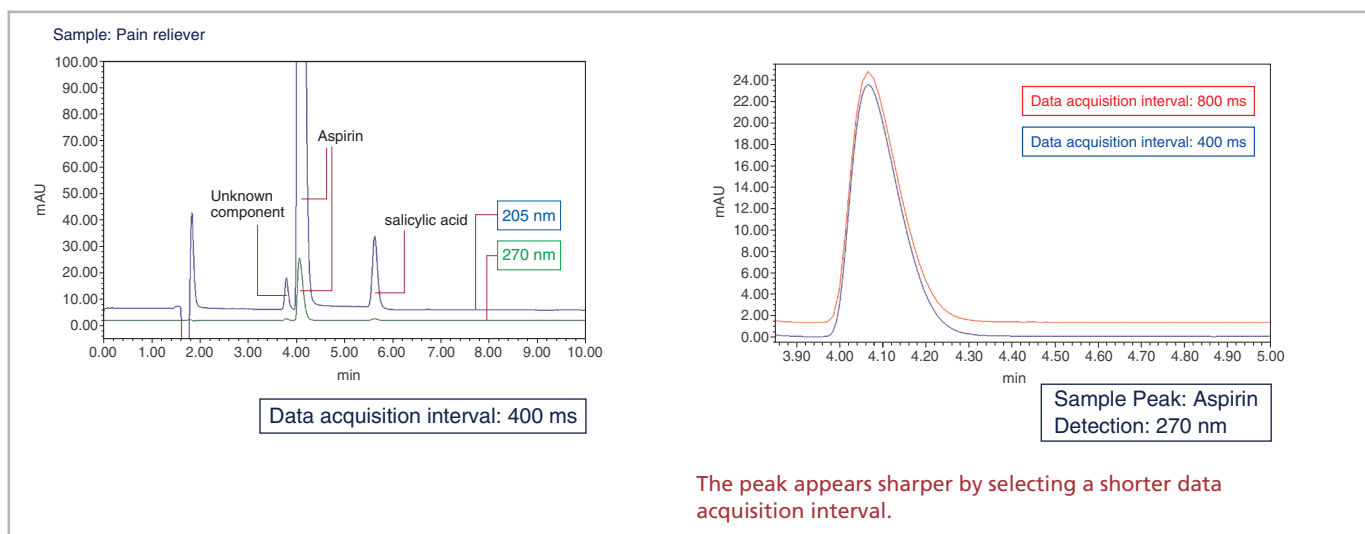

5440 Fluorescence Detector 5450 RI Detector



5440 Fluorescence Detector

High sensitivity with an S/N ratio of 900 or higher in water Raman

The detector incorporates low-light loss optics featuring a baseline method) in water Raman.

Thermostat flow cell

Thermostat controlled flow cell of ambient temperature changes is available. You can use

Fluorescence detector with a variable slit

The spectrometer slit on the fluorescence detector can be set between 15 nm and 30 nm. For high-sensitivity analyses, use the 30 nm slit.

Automatic wavelength check using a built-in Hg lamp

Similar to the UV detector, the 254 nm bright line from the Hg lamp can be used to perform wavelength checks in the UV region that is often used in HPLC analyses.



5450 Refractive Index (RI) Detector

Short stabilization time

The RI detector permits the start of measurement about 1 hour after it is powered on.

Flow cell with variable temperature setting


The flow cell in the RI detector can be set to a variable temperature setting.



Chromaster

Introducing a new mass detector from Hitachi designed for HPLC users

5610 MS Detector

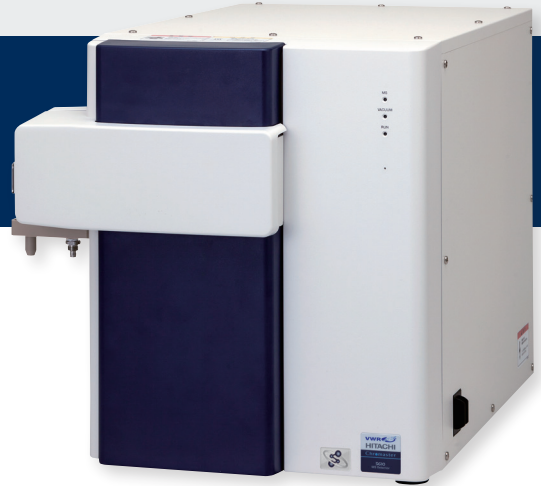

Optimized for qualitative analysis


When measuring samples that do not absorb UV light or using UV spectra alone, additional information provided by mass spectra can improve the reliability of qualitative analysis.

Ease of use

Operability on par with standard HPLC systems. The during maintenance.


Compact design for small footprint

The space-saving footprint is equivalent to that of a standard HPLC system. The required power source is 200 to 240 VAC, As the system is designed to use a minimum amount of N2 gas

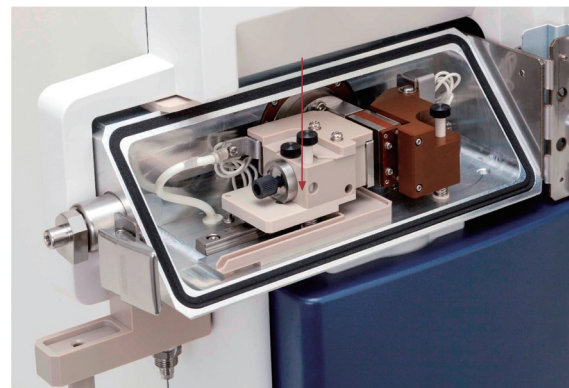


Application examples

Measurement of components that do not absorb UV light

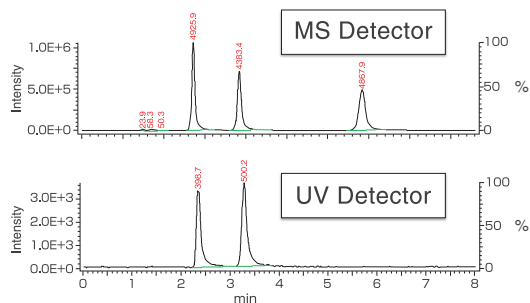


Additional information m/z data

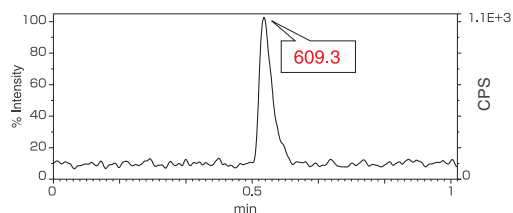

The m/z data can be displayed on the total ion chromatogram
*A software program for detector control and data analysis is supplied with 5610 MS Detector.


Improved data reliability

UV spectrum

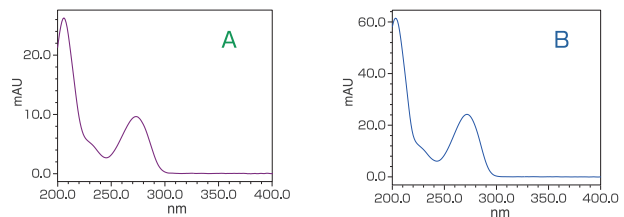

UV spectra alone cannot distinguish between A and B

Mass spectrum

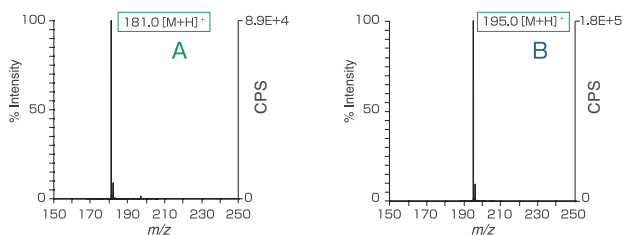

Additional mass spectra can help distinguish between A and B

Organizer



Organizer capable of accommodating various solvent bottles

The organizer can accept the simultaneous mounting of the following solvent bottles.

Organizer also doubles as a power supply module

The organizer, which is also a power supply module, supplies power to one pump, one autosampler, one detector (one UV detector, one UV-VIS detector, one Diode array detector or one RI detector), and one interface control board. Additional modules require an (optional) AC adapter or AC input.

Example

1	3,785 l (U.S. gallon bottle) × 2 + 500 ml × 2
2	3 l (Japanese gallon bottle) × 2 + 500 ml × 2
3	2,5 l (EU gallon bottle) × 2 + 500 ml × 3
4	1 l bottle × 5 + 500 ml × 2

(1) to (3) are for isocratic, 2-liquid gradient analysis, designed for use in quality control operations.

(4) is for method development.





Chromaster

Intuitive operation via unique touch panel

GUI Controller

Integrated module control

- A color LCD monitor (5,7-inch color TFT display with LED back light) and a touch panel make for easy viewing and simple operation.
- Modules^{*1, *2} can be controlled from this controller.
- Up to 10 programs involving a timer function, pre-analysis system tasks (Wakeup), and post-analysis system tasks (Sleep) can be created^{*1, *2, *3}.
- The GUI controller can control three pumps (of which one is isocratic) (useful for building pre-treatment systems, such as deproteinization).
- The GUI controller enables you to check the status of consumables usage on units^{*1, *2} that are connected to the system.



Main settings in the modules

Pump ^{*1, *2} Needle washing, rinse-port washing, and syringe purging
Autosampler: Needle washing, rinse-port washing, and syringe purging
Oven ^{*2} Temperature control and temperature stability
Detector ^{*1, *2} Temperature control and temperature stability

*1: Exclusive of 5610 MS detector *2: Exclusive of 6310 column oven *3: Exclusive of 5280 autosampler

Wakeup (automatic pre-analysis tasks) and Sleep (automatic post-analysis tasks) programs

Automatic system wakeup and sleep from GUI

- In conditioning, 10 programs for each pre-analysis system tasks (Wakeup) and post-analysis system tasks (Sleep) can be created in optional combination of settings.
- For Wakeup program ending time, you can specify any time up to three days later or after the end of a continuous analysis run. The automation of system stand-by can reduce the amount of time required to make preparations for an analysis run.



Controller that pairs with one module

- for modules that require stand-alone operations.
- The large button size and a wide pitch enhance the ease of operation.
- Instructions received from the autosampler.

* Standard accessory for 5450 RI detector
 * Not included with 5430 diode array detector, 5610 MS detector, and 6310 column oven



* Separate software for the instrument control and data processing is required when using 6310 column oven.


User oriented, convenient and smart system design

- Most optional accessories are internally mounted to reduce HPLC system height. The handle located on the front side of the organizer moves vertically for easy access to solvent bottles.
- With a module width of 340 mm*¹ and a depth of 440 mm, the system provides space savings.
 - *1 Exclusive of the column oven.
- Module operations and the replacement of consumable and maintenance parts can be performed from the front side.
- With attention to detail on the housing of tubes and wires, the system keeps tubes from getting tangled up, ensures the ease of replacement, and provides adequate seismic stability. In addition to incorporating these practical considerations, the system features a sleek, attractive appearance.



Front access
(Example: replacing lamps)



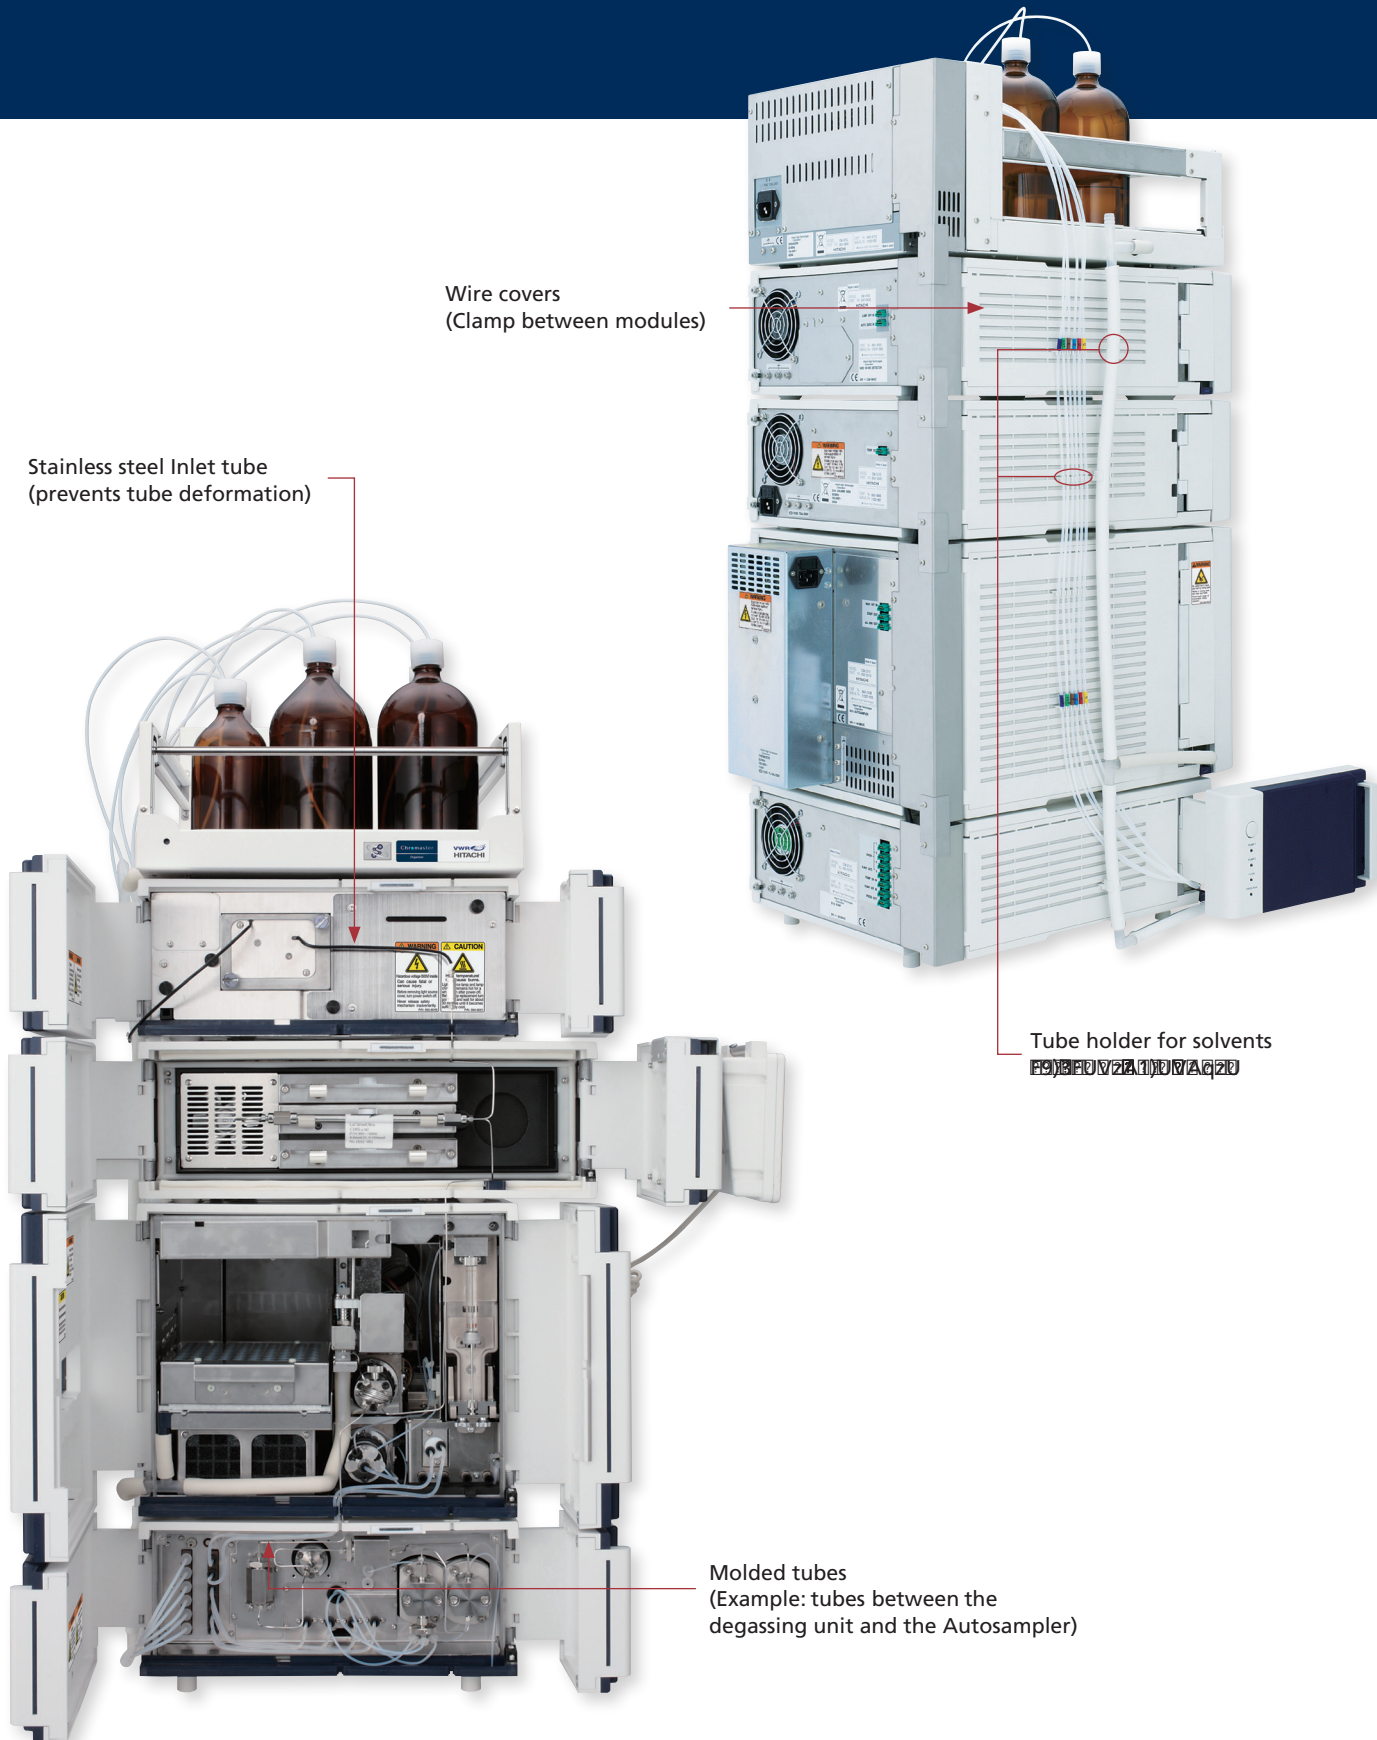

Stainless steel Inlet tube
(prevents tube deformation)

Wire covers
(Clamp between modules)

Tube holder for solvents
P9380V2A1D07A020

Molded tubes
(Example: tubes between the
degassing unit and the Autosampler)

Chromaster[®] Modules

5110/5160 Pump 5110/5160 Pump with Auto-purge valve



Main optional accessories

Low-pressure Gradient Unit for 5110/5160 (with Conventional Mixer)	Manual Injector Holder	THF kit for 5110/5160*
6 - channel Degassing unit (480 μ l)	Column Holder	THF kit for 5110/5160 with AP valve*
Plunger Washing Pump	UI Pad for 5110/5160	THF kit for Low Gr unit for 5110/5160
Conventional Mixer (700 μ l)	AC adapter (150 W)	Low dispersion piping kit
Semi - micro Mixer (200 μ l)	Hexane 6-channel Degassing unit for 5110/5160	
Dynamic Mixer (2,000 μ l)	Hexane Check Valve Set for 5110	

* Withstand pressure 40 MPa

5310/6310 Column Oven



Main optional accessories

Column management system for 5310
2-position, 6-port valve for 5310*
3 column selector valve for 5310*
UI Pad for 5310
MEM Column Fitting for 6310
6 column selector valve for 6310

* Withstand pressure 40 MPa

5610 MS Detector



Main optional accessories

System piping kit

Control and analysis software is standard accessory.

5410 UV Detector



5420 UV-VIS Detector



5430 Diode Array Detector



Main optional accessories

Analog signal output unit (1ch)	Semi-micro flow cell unit for 5410/5420
UI Pad for 5410/5420	HP SM flow cell unit for 5410/5420
AC adapter (150 W)	Preparative flow cell unit for 5410/5420
Thermo cell for 5410/5420	Thermo cell control unit for 5410/5420

Main optional accessories

2ch Analog signal output unit for 5430
AC adapter (150 W)
Semi-micro flow cell unit for 5430
HP SM flow cell unit for 5430
Preparative flow cell unit for 5430
Thermo cell for 5430
Thermo cell control unit for 5430

Organizer



Main optional accessories

Can be used as a cabinet that holds solvent bottles
Supplies power to one pump, one autosampler, one detector (one UV detector, one UV-VIS detector, one Diode array detector or one RI detector), and one interface control board



Chromaster

5260/5280 Autosampler 5260/5280 Autosampler with Thermostat/Thermo Unit



5260/5280 optional accessories

Sample rack (4 ml × 72)	Thermostat micro plate rack (2 pcs)	AC adapter (150 W)
Thermostat rack (4 ml × 72)	Syringe kit (70 µl, 700 µl)	Hexane kit for 5210/5260
Sample rack (1 ml × 195)	Sample loop kit (5 µl, 1 µl)	Hexane kit for 5210/5260*
Thermostat rack (1 ml × 195)	2-channel Degassing unit (250 µl / ch)	
Micro plate rack (2 pcs)	UI Pad for 5260	* Withstand pressure 40 MPa

5280 optional accessories

Sample rack (4 ml × 128)	Thermo unit micro plate rack (3 pcs)	AC adapter (150 W)
Thermo unit rack (4 ml × 128)	Syringe kit (500 µl, 1 ml)	
Micro plate rack (3 pcs)	UI Pad for 5280	

5440 Fluorescence Detector

Main optional accessories

- Analog signal output unit (1ch)
- UI Pad for 5440
- Thermo cell for 5440
- Thermo cell control unit for 5440



5450 RI Detector

Main optional accessories

- AC adapter (150 W)



Interface control board (IFC board)

Interface box



Front side



Back side

Main optional accessories

- Interface control board (IFC board) (for installing a 5260 autosampler)
- Interface box (S) (with an IFC board)
- Interface box (L) (with IFC board and one AID board)

The Photo is an Interface box(L)with another AID board installed.
For systems that do not have an organizer, AC adapter (60 W) is required.

GUI Controller



Main optional accessories

- GUI Controller – Interface Control Board is required.

AC adapter

Main optional accessories

- AC adapter (60 W) (for IFC board/Interface box)
For systems that do not have an organizer
- AC adapter (150 W)
(for Pump, Autosampler and UV/UV-VIS/Diode array detector/RI detector)
For systems that do not have an organizer

Main specifications

5110/5160 Pump	5110	5160
Item	Specifications	
Pumping system	Dual plunger reciprocating pump system Series connection, pulsation elimination system	
Operating flow rate range	0,001 to 9,999 ml/min	0,001 to 5,000 ml/min
Maximum operating pressure	40 MPa (0,001 to 5,000 ml/min) 20 MPa (5,001 to 9,999 ml/min)	60 MPa (0,001 to 2,500 ml/min) 30 MPa (2,501 to 5,000 ml/min)
Flow rate accuracy	± 1,0 % or ± 2,0 µl / min, whichever is greater, (0,010 to 5,000 ml/min, under a specified condition)	± 0,5 % or ± 2,0 µl / min, whichever is greater, (0,010 to 2,500 ml/min, under a specified condition)
Flow rate precision	SD0.02 min or RSD0.075 %, whichever is greater, under a specified condition	
Materials of wetted parts	Stainless steel, ruby, sapphire, ceramics, PTFE, carbon-containing PTFE, PEEK*1 (Auto-purge valve unit)	Stainless steel, ruby, sapphire, ceramics, PTFE, carbon-containing PTFE, Vespel*2 (Polyimide resin) (Auto-purge valve)
Functions of GLP	(Total flow rate display (Double speed error (Changeover number of times of the proportioning valve (Running time of the dynamic mixer (Changeover number of times of the auto purge valve (Operating time of the plunger wash pump	
Dimensions and weight	340 (W) × 440 (D) × 140 (H) mm, Approx.16 kg	
Power supply and Power consumption	DC 24 V, 4 A (Maximum) 96 W (power supply from organizer)	
Others	Pumps are available with and without an auto-purge valve.	

Loop reservoir (optional)	
Item	Specifications
Number of mixed solvents	Up to 4
Mixing system	Electromagnetic valve open/close time control system
Composition accuracy	±0,5 % (5 to 95 %)
Flow rate range recommended for analysis	0,4 to 1,8 ml/min

5260 / Autosampler 260	5280	
Item	Specifications	
Sample capacity	120 × 1,5 ml (Standard)	200 × 1,5 ml (Standard)
Sample injection system	Loop injection method (Cut injection, All volume injection, Full loop injection method)	Direct injection method
Syringe volume	175 µl (standard) (option syringe available)	100 µl (standard) (option syringe available)
Sample injection volume	0,1 to 50 µl (100 µl loop) (standard) (200 µl loop) (option)	0,1 to 50 µl (100 µl loop) (standard) (200 µl loop) (option)
Injection volume precision	-0,2 % RSD (10 µl, cut injection method) -0,25 % RSD (5 µl, cut injection method) -0,9 % RSD (1 µl, cut injection method) -1,0 % RSD (1 µl, All volume injection method) -0,2 % RSD (5 µl, full loop method)	-0,2 % RSD (10 µl, standard syringe) -0,25 % RSD (5 µl, standard syringe) -0,9 % RSD (1 µl, standard syringe) -1,0 % RSD (1 µl, standard syringe) -0,2 % RSD (5 µl, standard syringe)
Carry-over	-0,003 % (cut method)	-0,003 % RSD (under a specified condition)
Materials of wetted parts	Stainless steel, Vespel*2, fluoro-resin, PP, EPDM, PEEK*1, UHMWPE	Stainless steel, PEEK*1, fluoro-resin, PP, EPDM, Vespel*2, UHMWPE, DLC
Withstand pressure	60 MPa	60 MPa
Temperature setting range	1 to 45 °C (1 °C step), using Autosampler with a thermostat	1 to 35 °C (1 °C step), using Autosampler with a thermo unit
Temperature control range	[RT-21 °C] to [RT+25 °C] and range of the temperature setting (with a vial) [RT-15 °C] to [RT+20 °C] and range of the temperature setting (with a MTP) (using Autosampler with thermostat) An autosampler (with a thermostat) should be selected for the analysis of thermally sensitive samples.	4 to (RT - 5) °C at ambient temperature of 15 to 25 °C and humidity of 60 %
Functions of GLP	a) Injection port seal (Injection valve seal (Syringe valve seal (Syringe (Wash pump operation time	(Injection port seal (Injection valve seal (Syringe valve seal (Syringe
Dimensions and weight	340 (W) × 440 (D) × 280 (H) mm, approx. 24 kg (with thermostat, 340 (W) × 500 (D) × 280 (H)mm, approx. 29 kg)	340 (W) × 520 (D) × 320 (H) mm, approx. 23 kg (with thermo unit, approx. 26 kg)
Power supply and Power consumption	DC24 V, 4 A (maximum)/96 W (power supply from organizer) AC100 to 240 V (50 Hz/60 Hz) 110 VA (using Autosampler with thermostat)	DC24 V, 4 A AC100 to 240 V ±10 % (50 Hz/60 Hz) 110 VA (using Autosampler with thermo unit)
Others	Autosamplers are available with and without a thermostat.	Autosamplers are available with and without a thermo unit.

5310 / Oven 310	6310	
Item	Specifications	
Temperature control system	Heating/Cooling block + air circulation system	
Temperature setting range	1 to 85 °C (1 °C step)	1 to 90 °C (1 °C step)
Temperature control range	[Ambient temperature -15 °C] to [Ambient temperature +60 °C] and range of the temperature setting	[Ambient temperature -15 °C] to [Ambient temperature +75 °C] and within temperature setting range
Temperature accuracy	± 1,0 °C (20 to 85 °C, part of Pre-heat)	± 0,5 °C (20 to 50 °C), ± 1,0 °C (51 to 90 °C), after calibration
Temperature control precision	SD - 0,2 °C (under a specified condition)	± 0,1 °C (20 to 90 °C)
Time program functions	• Temperature setting • Switching valve (changing of position)	• Temperature setting • Switching valve (changing of position)
Functions of GLP	Recording of the changeover number of times and exchange dates of the optional changeover valve.	
Column capacity	300 mm × 3 (maximum)	
Dimensions and weight	410 (W) × 440 (D) × 140 (H) mm, Approx.13kg	165 (W) × 515 (D) × 689 (H) mm (Legs are not included), approx. 25 kg
Power supply and Power consumption	AC100 to 240 V (50 Hz/60 Hz)/230 VA (with optional valves) The Organizer and the AC adaptor are not necessary.	AC100 to 240 V (50 Hz/60 Hz)/300 VA The Organizer and the AC adaptor are not necessary.



5410 Detector	
Item	Specifications
Optical system	Double-beam ratio photometric system
Light source	D2 lamp, Hg lamp for checking wavelength
Wavelength range	190 nm to 600 nm
Wavelength accuracy	±1 nm
Spectral bandwidth	6 nm
Noise	-0,5 × 10 ⁻⁵ AU at 250 nm
Drift	-1,0 × 10 ⁻⁴ AU/h at 250 nm
2-wavelength measurement	2 wavelengths in wavelength regions 190 to 350 nm and 351 to 600 nm, respectively (Minimum wavelength interval 5 nm, max. wavelength interval 160 nm with data sampling period set at 400 ms)
Response	0,01 sec, 0,02 sec, 0,05 sec, 0,1 sec, 0,5 sec, 1 sec, 2 sec
Materials of wetted parts	Quartz glass, fluoro-resin, stainless steel
Functions of GLP	(D2 lamp/Hg lamp lighting time, lighting number of times, and replacement record) (Key lock) (D2 lamp energy check and D2 lamp wavelength check) (Hg lamp wavelength check)
Flow cell	13 µl (Optical path length 10 mm)
Thermostatically flow cell	Optional, environmental temperature
Dimensions and weight	340 (W) × 440 (D) × 140 (H) mm, approx. 14 kg
Power supply and Power consumption	DC24 V, 2,5 A (maximum)/60 W (power supply from organizer) Please purchase the AC adaptor (150 W) when there is no organizer.

5430 Detector	
Item	Specifications
Detection type	1,024 bit PDA
Light source	D2 lamp, W lamp, Hg lamp for checking wavelength
Wavelength range	190 to 900 nm
Wavelength accuracy	±1 nm
Noise	-0,5 × 10 ⁻⁵ AU at 250 nm condition
Drift	-0,4 × 10 ⁻³ AU/h at 250 nm condition
Response	0,01 sec, 0,02 sec, 0,05 sec, 0,1 sec, 0,5 sec, 1 sec, 2 sec
Slit type	1 nm/4 nm (variable)
Materials of wetted parts	Quartz glass, fluoro-resin, stainless steel
Functions of GLP	(D2 lamp/W lamp/Hg lamp lighting time, lighting number of times, and replacement record) (D2 lamp energy check) (W lamp energy check) (Hg lamp wavelength check) (D2 lamp wavelength check)
Flow cell	13 µl (optical path length 10 mm)
Thermostat flow cell	Optional, environmental temperature
Dimensions and weight	340 (W) × 440 (D) × 140 (H) mm, approx. 14 kg
Power supply and Power consumption	DC24 V, 3,5 A (maximum)/84 W (power supply from organizer) Please purchase the AC adaptor (150 W) when there is no organizer

5450 Detector	
Item	Specifications
Refractive index range	1 to 1,75
Noise	-2,5 × 10 ⁻⁹ RIU
Drift	-0,2 × 10 ⁻⁶ RIU/h
Time constant	0,05 sec, 0,1 sec, 0,25 sec, 6 sec
Temperature control range	OFF, and 30 to 50 °C
Materials of wetted parts	Stainless steel, fluoro-resin, quartz glass, sapphire (Al2O3)
Dimensions and weight	340 (W) × 440 (D) × 140 (H) mm, excluding projections, approx. 13 kg
Power supply and Power consumption	DC24 V, 5 A (maximum)/120 W (maximum) (power supply from organizer) Please purchase the AC adaptor (150 W) when there is no organizer.

5610 MS Detector	
Item	Specifications
Measurement mass range (m/z)	20 to 1,000
Ion source	Electrospray ionization (ESI)
Dimensions and Weight	440(W) x 610(D) x 430(H) mm / approx. 51 kg
Power supply and Power consumption	AC 200 to 240 V (50 Hz/60 Hz)/1,000 VA
N2 gas usage	Max flow rate 3,4 l/min, pressure 300 ± 20 kPa

5420 - Detector	
Item	Specifications
Optical system	Double-beam ratio photometric system
Light source	D2 lamp, W lamp, Hg lamp for checking wavelength
Wavelength range	190 nm to 900 nm
Wavelength accuracy	±1 nm
Spectral bandwidth	6 nm
Noise	-0,5 × 10 ⁻⁵ AU at 250 nm, 600 nm condition
Drift	-1,0 × 10 ⁻⁴ AU/h at 250 nm, 600 nm condition
2-wavelength measurement	2 wavelengths in wavelength regions 190 to 350 nm, 351 to 400 nm, 401 to 600 nm and 601 to 900 nm (D2&W mode) 2 wavelengths in wavelength regions 190 to 350 nm and 351 to 600 nm (D2 mode) 2 wavelengths in wavelength regions 380 to 600 nm and 601 to 900 nm (W mode) (Minimum wavelength interval 5 nm, max. wavelength interval 160 nm with data sampling period set at 400 ms)
Response	0,01 sec, 0,02 sec, 0,05 sec, 0,1 sec, 0,5 sec, 1 sec, 2 sec
Materials of wetted parts	Quartz glass, fluoro-resin, stainless steel
Functions of GLP	(D2 lamp/W lamp/Hg lamp lighting time, lighting number of times, and replacement record) (Key lock) (D2 lamp energy check and D2 lamp wavelength check) (W lamp energy check) (Hg lamp wavelength check)
Flow cell	13 µl (optical path length 10 mm)
Thermostatically flow cell	Optional, environmental temperature
Dimensions and weight	340 (W) × 440 (D) × 140 (H) mm, approx. 14 kg

5440 Detector	
Item	Specifications
Light source	Xe lamp, Hg lamp for checking wavelength
Wavelength range	Ex: 200 to 850 nm Em: 250 to 900 nm (change photomultiplier at 731 nm or more)
Wavelength accuracy	±3 nm
Response	0,01 sec, 0,02 sec, 0,05 sec, 0,1 sec, 0,5 sec, 1 sec, 2 sec
Spectral bandwidth	Ex: 15 nm, Em: 15, 30 nm (variable)
Sensitivity	>900 S/N ratio of water raman (bandwidth 30 nm, Ex=350 nm, TC=2 s, baseline method, standard cell)
Materials of wetted parts	Quartz glass, fluoro-resin, stainless steel
Functions of GLP	(lamp energy check, (wavelength accuracy check, (lamp lighting time, lighting number of times, and replacement record)
Flow cell	Irradiation volume 12 µl
Thermostat flow cell	Optional, environmental temperature range: 4 to 30 °C
Dimensions and weight	340 (W) × 440 (D) × 280 (H) mm, approx. 25 kg
Power supply and Power consumption	AC100 to 240 V (50/60 Hz)/330 VA The Organizer and the AC adaptor are not necessary.

Organizer	
Item	Specifications
Output power	DC24 V, 450 W Supplies power to one pump, one autosampler, one detector (one UV detector, one UV-VIS detector, one diode array detector, or one RI detector), and one interface control board
Bottle capacity and the space	1,0 l bottle × 6 and 500 ml bottle × 3 (maximum), 314 (W) × 280,8 (D)mm
Dimensions and weight	340(W) × 420(D) × 200(H)mm, approx. 9 kg
Power supply and Power consumption	AC100 V to 240 V (50 Hz/60 Hz), 520 VA

*1 "PEEK" is a registered trademark of VICTREX PLC. in the European Union.

*2 Vespel: "VESPEL" is a registered trademark of E I Du Pont De Nemours and Company in Denmark and Switzerland.

HPLC system, Chromaster



All preconfigured systems (including detector) are delivered with all necessary cables and an interface board.

The VWR Hitachi Chromaster delivers highly reliable results. This is achieved with the high precision delivered by the pump, the low carry-over and high precision of the autosampler, the stability of the column oven and the sensitivity of the detectors.

cooperation. During this time, the robustness and reliability of the Hitachi HPLC instruments has helped to build and develop a strong partnership.

Chromaster key parameters:

- 600 bar (60 MPa) maximum operating pressure as standard with highly stable pulsation elimination system
- Very low carry-over autosamplers. Loop injection and direct injection available with peltier thermostatted sample racks
- Diode Array Detector, 1028 bit PDA with very low drift and noise
- Excellent gradient reproducibility
- Automatic wavelength using mercury lamp for UV, DAD and Fluorescence Detectors
- Unique touch screen user interface
- Drivers available for OpenLab® CDS, Chromeleon® 6.8 and 7.X, Empower3® and Clarity

brochure and product sheets.

Preconfigurations

Hi-Resolution Chromaster (High Performance)	pk	Cat. No.
Chromaster HPLC system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5430 diode array detector with high pressure 150 bar semi micro (3,2 µl, 5 mm) flow cell kit for low dispersion. Chromaster System Manager control and data acquisition software included. Suitable for use with smaller particle size columns for faster HPLC	1	903-0350
Chromaster HPLC system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5430 diode array detector with high pressure 150 bar semi micro (3,2 µl, 5 mm) flow cell kit for low dispersion. Chromaster System Manager control and data acquisition software included. Suitable for use with smaller particle size columns for faster HPLC	1	903-0336
Chromaster systems for use with standard columns	pk	Cat. No.
Chromaster HPLC system including 5160 quaternary gradient pump max. pressure 600 bar with manual purge valve and 6 channel degasser. 5260 autosampler with low carry-over loop injection and 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5410 variable wavelength UV detector with 13 µl, 10 mm flow cell. Chromaster System Manager control and data acquisition software included	1	903-0337
Chromaster HPLC system including 5160 quaternary gradient pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler and low carry-over loop injection 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5420 variable wavelength UV detector with 13 µl, 10 mm flow cell	1	903-0354
Chromaster HPLC system including 5160 quaternary gradient pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler and low carry-over loop injection 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5410 variable wavelength UV detector with 13 µl, 10 mm flow cell. Chromaster System Manager control and data acquisition software included	1	903-0396
Chromaster systems with Diode Array Detector (DAD)	pk	Cat. No.
Chromaster HPLC system including 5160 quaternary gradient pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5280 autosampler with 200 vial rack and direct injection with needle integrated into sample loop and 100 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5410 variable wavelength UV detector with 13 µl, 10 mm flow cell	1	903-0352
Chromaster HPLC system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5280 autosampler with 200 vial peltier cooled sample rack, direct injection with needle integrated into sample loop and 100 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5430 diode array detector with 13 µl, 10 mm cell	1	903-0353
Chromaster systems with Loop injection and DAD	pk	Cat. No.
Chromaster HPLC system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5430 diode array detector with 13 µl, 10 mm cell. Chromaster System Manager control software included	1	903-0593
Chromaster HPLC system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection 175 µl syringe. 5310 oven for max. 3 x 300 mm columns. 5430 diode array detector with 13 µl, 10 mm cell	1	903-0355
Chromaster manual injection system	pk	Cat. No.
Chromaster HPLC manual injection system including 5160 quaternary gradient pump max. pressure 600 bar with manual purge valve and 6 channel degasser. 7725I-188 Manual Injection Valve, 5410 variable wavelength UV detector with 13 µl, 10 mm flow cell	1	903-0363

Preconfigured wide port detector		
Description	pk	Cat. No.
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection. 5310 oven for max. 3 x 300 mm columns	1	903-0340
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with low carry-over loop injection and rack for 120 x 1,5 ml vials. 5310 oven for max. 3 x 300 mm columns	1	903-0341
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with manual purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection. 5310 oven for max. 3 x 300 mm columns	1	903-0342
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with manual purge valve and 6 channel degasser. 5260 autosampler with low carry-over loop injection and rack for 120 x 1,5 ml vials. 5310 oven for max. 3 x 300 mm columns	1	903-0343
Preconfigurable wide port detector		
Description	pk	Cat. No.
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5280 autosampler, peltier cooling with 200 vial rack and direct injection with needle integrated into sample loop and 100 µl syringe. 5310 oven for max. 3 x 300 mm columns	1	903-0356
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5280 autosampler with 200 vial rack and direct injection with needle integrated into sample loop and 100 µL syringe. 5310 Oven for max. 3 x 300 mm columns	1	903-0357
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with manual purge valve and 6 channel degasser. 5280 autosampler, peltier sample cooling with 200 vial rack and direct injection with needle integrated into sample loop and 100 µl syringe. 5310 oven for max. 3 x 300 mm columns	1	903-0358
Chromaster HPLC base system including 5160 quaternary pump max. pressure 600 bar with manual purge valve and 6 channel degasser. 5280 autosampler with 200 vial rack and direct injection with needle integrated into sample loop and 100 µl syringe. 5310 oven for max. 3 x 300 mm columns	1	903-0359
Preconfigurable narrow port detector		
Description	pk	Cat. No.
Chromaster HPLC base system for gel permeation chromatography including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with peltier thermostated rack to 45 °C and low carry-over loop injection. 5310 Oven for max. 3 x 300 mm columns. THF Resistant parts included	1	903-0338
Chromaster HPLC base system for normal phase chromatography including 5160 quaternary pump max. pressure 600 bar with auto purge valve and 6 channel degasser. 5260 autosampler with low carry-over loop injection. 5310 Oven for max. 3 x 300 mm columns with high temperature stability. Hexane/Heptane resistant parts included	1	903-0339

Main modules		
Description	pk	Cat. No.
Chromaster HPLC 5410 UV variable wavelength detector	1	903-0524
Chromaster HPLC 5420 UV-VIS variable wavelength detector	1	903-0525
Chromaster HPLC 5430 diode array detector without flow cell	1	903-0597
Chromaster HPLC 5440 fluorescence detector	1	903-0527
Chromaster HPLC 5440 standalone fluorescence detector including UI pad, analogue output, detector signal cable and power unit	1	903-0360
Chromaster HPLC 5450 refractive index detector	1	903-0528
Chromaster 5610 mass selective detector, including control software (MSD System Manager, English Version)	1	903-0397
ELSD 90 HPLC low temperature evaporative light scattering detector, 230 V, EU-plug	1	903-0271
Chromaster HPLC 5110 pump with manual purge valve. 400 bar max. operating pressure (9,99 ml/min max. flow rate)	1	903-0500
Chromaster HPLC 5110 pump with auto-purge valve. 400 bar max. operating pressure (9,99 ml/min max. flow rate)	1	903-0501
Chromaster HPLC 5160 pump with manual purge valve. 600 bar max. operating pressure (4,99 ml/min max. flow rate)	1	903-0554
Chromaster HPLC 5160 pump with auto-purge valve. 600 bar max. operating pressure (4,99 ml/min max. flow rate)	1	903-0555
Chromaster HPLC 5260 autosampler with 175 µl syringe. 600 bar max. operating pressure	1	903-0556
Chromaster HPLC 5260 autosampler with thermostat and 175 µl syringe. 600 bar max. operating pressure	1	903-0557
Chromaster HPLC 5280 autosampler with peltier cooling unit and 100 µl syringe. 600 bar max. operating pressure	1	903-0345
Chromaster HPLC 5280 autosampler with 100 µl syringe. 600 bar max. operating pressure	1	903-0344
Chromaster HPLC 5310 column oven for max. 3 x 300 mm columns	1	903-0520
Chromaster HPLC 6310 column oven for max. 6 x 100 mm columns or max. 3 x 300mm columns	1	903-0361
Chromaster organiser for solvent placement and power supply	1	903-0537

Accessories		
Description	pk	Cat. No.
Chromaster HPLC low pressure quaternary gradient unit. Includes proportioning valves, conventional mixer and capillaries. For Chromaster HPLC 5110 and 5160 pumps	1	903-0562
Chromaster HPLC 6-channel degassing unit with 480 µl degassing chambers. For Chromaster HPLC 5110 and 5160 pumps	1	903-0503
Chromaster HPLC built-in dedicated mini pump for washing the plunger of the Chromaster HPLC 5110 and 5160 pumps	1	903-0563
Chromaster HPLC 6-channel hexane resistant degassing unit with 480 µl degassing chambers for use with both Chromaster HPLC 5110 and 5160 pumps	1	903-0567
Chromaster HPLC hexane resistant check valve for Chromaster HPLC 5110 and 5160 pumps	1	903-0559

HPLC control interfaces for Chromaster		
Description	pk	Cat. No.
Chromaster system manager software for method creation, data acquisition, chromatograph data processing, DAD data processing and report generation	1	906-0144
OpenLAB CDS EZChrom Edition including 1 year Software Maintenance Agreement + Hitachi LC Control	1	906-0145
OpenLAB CDS EZChrom Edition including 1 year Software Maintenance Agreement + Hitachi LC Control + Hitachi DAD	1	906-0146
Chromaster HPLC Interface Control Board for Chromaster system control. USB cable and e-line cable (0,5 m) included. Built into the autosampler upon installation in laboratory. If no autosampler is used, then the interface box (S) must be ordered instead	1	903-0545
Chromaster HPLC graphical user interface (GUI) touch screen controller for Chromaster 5000 series for integrated module control	1	903-0546

PC for software installation		
Description	pk	Cat. No.
Dell™ PC 64Bit/8Gb with Intel™ i5 Quad Core Chipset. Includes Dell™ mouse and international keyboard. 12 MUI languages preloaded. Three years Dell™ Warranty Next Business Day On Site plus two year LabService guarantee. Dell™ monitor 20" wide is included"	1	906-0210

Fr a c t ó l o i n é (ð é w)		
Description	pk	Cat. No.
Foxy R1, stand-alone package, includes diverter valve and rack for 18 mm Ø ext. tubes, interface and remote cable, E-DIO cable, flow rates up to 25 ml/min (with 1/16" outlet tubes)	1	905-0533

Control licences for Chromaster with existing software set-up		
Description	pk	Cat. No.
Chromaster Driver control licence for Waters Empower3®	1	906-0156
Chromaster control licence for Chromeleon® 6.8	1	906-0185
Chromaster control licence for Chromeleon® 7.X	1	906-0186
OpenLab™ CDS EZChrom edition licence for additional Hitachi HPLC with Diode Array on the same PC	1	906-0148
OpenLab™ CDS EZChrom edition licence for additional Hitachi HPLC on the same PC	1	906-0147

Accessories			
Description	For	pk	Cat. No.
Chromaster HPLC user interface keypad. Mounting parts included	Chromaster HPLC 5110 and 5160 pumps	1	903-0540
Chromaster HPLC user interface keypad. Mounting parts included	Chromaster HPLC 5260 autosamplers (built into the autosampler upon installation in laboratory)	1	903-0541
Chromaster HPLC user interface keypad. Mounting parts included	Chromaster HPLC 5310 column ovens (built into the column oven upon installation in laboratory)	1	903-0542
Chromaster HPLC user interface keypad. Mounting parts included	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors (built into the detector upon installation in laboratory)	1	903-0543
Chromaster HPLC user interface keypad. Mounting parts included	Chromaster HPLC 5440 fluorescence detectors (built into the detector upon installation in laboratory)	1	903-0544
Pump accessories			
Description	For	pk	Cat. No.
Chromaster HPLC dynamic mixer 2000 µl	Chromaster HPLC 5110 and 5160 pumps (built into the pump upon installation in laboratory)	1	903-0564
Chromaster HPLC 200 µl semi-micro mixer for flow rates of 0,4 ml/min or less	Chromaster HPLC 5110 and 5160 pumps (built into the pump upon installation in laboratory)	1	903-0507
Chromaster HPLC 700 µl static mixer for conventional use with flow rates between 0,4 and 1,8 ml/min	Chromaster HPLC 5110 and 5160 pumps (built into the pump upon installation in laboratory)	1	903-0565
Chromaster HPLC adaption kit for THF (max pressure 400 bar)	Chromaster HPLC 5110 and 5160 pumps with manual purge valve (built into the pump upon installation in laboratory)	1	903-0568
Chromaster HPLC adaption kit for THF (max pressure 400 bar)	Chromaster HPLC 5110 and 5160 pumps with autopurge valve (built into the pump upon installation in laboratory)	1	903-0569
Chromaster HPLC THF resistant Vespel® packing	Chromaster conventional mixer for use up to 400 bar	1	903-0570
Chromaster HPLC manual injection set	Chromaster configuration without autosampler	1	903-0362
Autosampler accessories			
Description	For	pk	Cat. No.
Chromaster HPLC sample rack for 120 × 1,5 ml sample vials. Supplied as standard with the 5260 autosamplers	Chromaster HPLC 5260 autosamplers	1	903-0511
Chromaster HPLC sample rack for 72 × 4 ml sample vials	Chromaster HPLC 5260 autosamplers	1	903-0512
Chromaster HPLC sample rack for 195 × 1 ml sample vials. Rack for ambient use	Chromaster HPLC 5260 autosamplers	1	903-0513
Chromaster HPLC sample rack for 2 × 96-well or 384-well micro titre plates	Chromaster HPLC 5260 autosamplers	1	903-0514
Chromaster HPLC sample rack for 120 × 1,5 ml sample vials. Supplied as standard with the the 5260 thermostat autosamplers	Chromaster HPLC 5260 autosamplers	1	903-0406
Chromaster HPLC sample rack for 72 × 4 ml sample vials	Chromaster HPLC 5260 autosamplers with thermostat	1	903-0516
Chromaster HPLC sample rack for 195 × 1 ml sample vials	Chromaster HPLC 5260 autosamplers with thermostat	1	903-0517
Chromaster HPLC sample rack for 2 × 96-well or 384-well microtitre plates	Chromaster HPLC 5260 autosamplers with thermostat	1	903-0518
Chromaster HPLC 70 µl syringe kit	Chromaster HPLC 5260 autosamplers	1	560-0173
Chromaster HPLC 700 µl syringe kit	Chromaster HPLC 5260 autosamplers	1	903-0560
Chromaster HPLC 3000 µl syringe kit	Chromaster HPLC 5260 autosamplers	1	903-0596
Chromaster HPLC sample loop kit (5 µl)	Chromaster HPLC 5260 autosamplers	1	903-0573
Chromaster HPLC sample loop kit (10 µl)	Chromaster HPLC 5260 autosamplers	1	903-0574
Chromaster HPLC sample loop kit (20 µl)	Chromaster HPLC 5260 autosamplers	1	903-0575
Chromaster HPLC sample loop kit (100 µl)	Chromaster HPLC 5260 autosamplers	1	903-0576
Chromaster HPLC sample loop (200 µl)	Chromaster HPLC 5260 autosamplers	1	903-0577
Chromaster HPLC sample loop (1000 µl)	Chromaster HPLC 5260 autosamplers	1	903-0561
Chromaster HPLC sample loop (4000 µl)	Chromaster HPLC 5260 autosamplers	1	903-0578
Chromaster HPLC 2-channel degassing unit. Only needed if pump degasser is not used	Chromaster HPLC 5260 autosamplers (built into the autosampler upon installation in laboratory)	1	903-0519
Chromaster HPLC hexane resistant autosampler washing pump	Chromaster HPLC 5260 autosamplers	1	903-0571
Chromaster HPLC THF resistant autosampler kit	Chromaster HPLC 5210 autosamplers (built into the autosampler upon installation in the laboratory)	1	903-0572




Accessories			
Column oven accessories	For	pk	Cat. No.
Chromaster HPLC 3-column selection valve. Pressure stability to 345 bar. For 1/16" capillaries. Power unit, control board and tubes are included. One valve per oven only	Chromaster HPLC 5310 column ovens (built into the column oven upon installation in laboratory)	1	903-0521
Chromaster HPLC 2-position, 6-port valve. Power unit, control board and tubes are included	Chromaster HPLC 5310 column oven (built into the column oven upon installation in laboratory)	1	903-0522
Chromaster HPLC 6 column selector Rheodyne® valve	for Chromaster HPLC 6310 oven	1	903-0351
Chromaster HPLC column management system. Three column electronic data tags are included	Chromaster HPLC 5310 column oven (built into the column oven upon installation in laboratory)	1	903-0523
Chromaster HPLC column holder	Chromaster HPLC use when an oven is not ordered (built into the detector upon installation in laboratory)	1	903-0566
Detector accessories	For	pk	Cat. No.
Chromaster HPLC thermo cell. Flow cell control unit for 5410 UV detector and 5420 UV-VIS detector is also required	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors (built into the detector upon installation in laboratory)	1	903-0529
Chromaster HPLC thermostat cell control unit. Necessary for thermo cell for 5410 UV detectors and 5420 UV-VIS detectors	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors (built into the detector upon installation in laboratory)	1	903-0535
Chromaster HPLC high pressure semi-micro flow cell, 150 bar, 3,2 µl, 5 mm	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors	1	903-0581
Chromaster HPLC preparative flow cell, 150 bar, 3,2 µl, 5 mm pressure resistance 1MPa	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors	1	903-0583
Chromaster HPLC standard flow cell	Chromaster HPLC 5430 diode array detectors (built into the detector upon installation in laboratory)	1	903-0320
Chromaster HPLC thermo cell. The thermostat cell control unit for 5430 diode array detector is also required	Chromaster HPLC 5430 diode array detectors (built into the detector upon installation in laboratory)	1	903-0530
Chromaster HPLC thermostat cell control unit. Necessary for thermo cell for 5430 diode array detector	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors (built into the detector upon installation in laboratory)	1	903-0536
Chromaster HPLC high pressure semi-micro flow cell, 150 bar, 3,2 µl, 5 mm	Chromaster HPLC 5430 diode array detectors	1	903-0584
Chromaster HPLC preparative flow cell, 150 bar, 3,2 µl, 5 mm pressure resistance 1MPa	Chromaster HPLC 5430 diode array detectors	1	903-0586
Chromaster HPLC thermostat flow cell. Thermostat flow cell control unit for 5440 fluorescence detectors is also required	Chromaster HPLC 5440 fluorescence detectors (built into the detector upon installation in laboratory)	1	903-0532
Chromaster HPLC thermostat flow cell control unit. For use with thermostat flow cell for 5440 fluorescence detectors	Chromaster HPLC 5440 fluorescence detectors (built into the detector upon installation in laboratory)	1	903-0533
Chromaster HPLC interface box (L) with Interface Control Board (IFCB), USB-analogue input device (AID). AC adapter (60 W) is required	Chromaster HPLC systems without autosampler	1	903-0547
Chromaster HPLC interface box (S). AC adapter (60 W) is required	Chromaster HPLC systems without autosampler	1	903-0548
Chromaster HPLC USB-analogue input device. Maximum 2 USB-AID allowed per system. Interface Control Board is required	Chromaster HPLC with 1 channel for analogue signal acquisition for Chromatography Data System	1	903-0549
Chromaster HPLC 2-channel analogue signal output unit	Chromaster HPLC 5430 diode array detectors (built into the detector upon installation in laboratory)	1	903-0531
Chromaster HPLC 1-channel analogue signal output unit	Chromaster HPLC 5410 UV detectors, 5420 UV-VIS detectors and 5440 fluorescence detectors (built into the detector upon installation in laboratory)	1	903-0534
Additional accessories	For	pk	Cat. No.
Chromaster HPLC adaptation plate	Chromaster HPLC assembling a LaChrom Elite® or LaChromUltra™ module into the configuration	1	903-0588
Chromaster HPLC tubing kit. Includes tubing and cables	Chromaster HPLC system in a two tower configuration	1	903-0587
Chromaster HPLC AC adapter (150 W)	Chromaster HPLC 5110/5160 pumps, 5260 autosamplers, 5410 UV detectors, 5420 UV-VIS detectors, 5430 diode array detectors and 5450 refractive index detectors. When no organiser is used	1	903-0538
Chromaster HPLC AC adapter (60 W)	Chromaster HPLC interface boxes (S) and (L)	1	903-0539
Low dispersion columns	For	pk	Cat. No.
Chromaster HPLC semi-micro flow cell kit including capillary set for low dispersion	Chromaster HPLC 5410 UV detectors and 5420 UV-VIS detectors	1	903-0589
Chromaster HPLC semi-micro flow cell kit including capillary set for low dispersion	Chromaster HPLC 5430 diode array detectors	1	903-0590



Clarity® is registered trademark of DataApex, Chromleon® (registered trademark of Thermo), Empower® (registered trademark of Waters), OpenLab CDS EE® (registered trademark of Agilent).

VWR tools for chromatographers

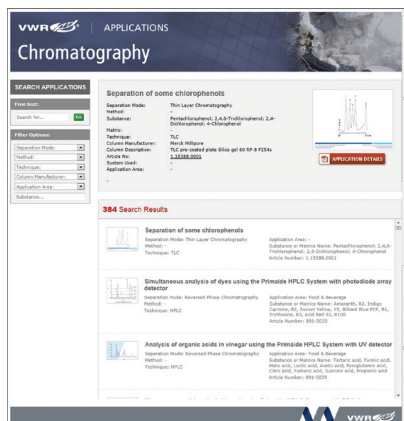

Application Services

Our applications chemists are highly experienced in the development and optimisation of HPLC and UHPLC methods, and provide the following services:

- Application advice
- Optimisation of existing methods
- Development of new methods
- Transfer of methods from standard HPLC systems to the ChromasterUltra Rs
- Scale-up of analytical methods to preparative HPLC
- Development and adaptation of special methods
- On-site application support
- Advice on method validation

VWR Chrom-Application library

Chromatography applications from VWR and our partners

- Free access to applications from VWR and partners
- Summary view and full download possibilities
- Every month new applications are added
- Application support from our own application labs
- Main columns used ready to order



Unique set of applications

Owing to our broad chromatography portfolio we can offer a variety of applications using the most suitable instruments, columns, chemicals and supplies. You can simply look at the overview or download the complete application. If you what your looking for, simply ask us!



Training

VWR can provide training on a number of topics:

Introduction to HPLC analysis; application tips, tricks and troubleshooting; operation of the VWR-Hitachi and other HPLC systems; training for different chromatography data systems along with other special software tools. Training courses can be held either at VWR headquarters or "in-house".

Software Support

A team of software specialists is on hand to support your chromatography data server systems supporting these systems through their life cycle.

NEW!

PC's and accessories for the chromatography lab

OpenLAB CDS EZChrom edition software pre-installed. Other PCs, accessories like monitors and printers, software such as Microsoft® XP plus IT services are available on request.



Chromatography Services

The VWR service department accompanies and supports you and your

customised service packages to optimise your results and keep costs down.

Installation and qualification

Our service engineers install and commission your chromatography system authorised Standard Operating Procedures and can be used to compile the necessary IQ, OQ and PQ documentation.

A team of software specialists is available to help you with all questions relating to data management; they install and validate your system either in an individual workstation or as part of your client-server system. Subsequently, they can monitor your systems over their entire lifespans.

We keep your system running

Regular expert maintenance keeps your analytical systems reliable and maintains the value of your investment. A maintenance contract increases the overall productivity of the system and generates more time for the user for other important tasks. Such a maintenance contract can be adapted to frequency of



8 GOOD REASONS FOR ESTABLISHING A SERVICE CONTRACT WITH VWR

- 1. Extended guarantee**
If on purchasing new equipment you take out a service contract, your guarantee automatically increases to three years.
- 2. Manufacturer's competence for optimal functionality**
Your apparatus will be regularly checked by competent service technicians certificated by the relevant manufacturer.
- 3. Calculable costs**
The costs involved for service and repair are completely calculable as they are covered by the contractual flat rate.
- 4. Reduction of operating costs**
The early recognition of wear and tear and technical defects prevents costly repairs, annoying downtime and prolongs the useful life of the equipment.
- 5. Priority treatment**
As a service contract customer, your repairs will be treated with priority.
- 6. Operability**
Regular servicing increases the operational safety of your equipment.
- 7. Minimum administrative effort and expense**
VWR coordinates and monitors your service requirements and carries them out at your convenience.
- 8. Original parts**
In carrying out service and repairs, only original parts are used.



Austria

VWR International GmbH
Graumanngasse 7
1150 Vienna
Tel.: +43 1 97 002 0
Fax: +43 1 97 002 600
Email: info@at.vwr.com

Belgium

VWR International bvba
Researchpark Haasrode 2020
Geldenaaksebaan 464
3001 Leuven
Tel.: 016 385 011
Fax: 016 385 385
Email: vwrbe@be.vwr.com

Czech Republic

VWR International s. r. o.
Veetee Business Park
8020127
710202082200
Tel.: +420 321 570 321
Fax: +420 321 570 320
Email: info@cz.vwr.com

Denmark

VWR - Bie & Berntsen
Transformervej 8
2860 Søborg
Tel.: 43 86 87 88
Fax: 43 86 87 90
Email: info@dk.vwr.com

Finland

VWR International Oy
Valimotie 9
00380 Helsinki
Tel.: 09 80 45 51
Fax: 09 80 45 52 00
87275@00072200

France

VWR International S.A.S.
Le Périgares – Bâtiment B
201, rue Carnot
94126 Fontenay-sous-Bois cedex
Tel.: 0 825 02 30 30 (0,18 € TTC/min)
Fax: 0 825 02 30 35 (0,18 € TTC/min)
Email: info@fr.vwr.com

Germany

VWR International GmbH
Hilpertstraße 20a
D - 64295 Darmstadt
Free-call: 0800 702 00 07
Fax: 0180 570 22 22*
Email: info@de.vwr.com
*0,14 €/Min. aus d. dt. Festnetz

Hungary

VWR International Kft.
Simon László u. 4.
4034 Debrecen
Tel.: (52) 521-130
Fax: (52) 470-069
Email: info@hu.vwr.com

Ireland / Northern Ireland

VWR International Ltd /
438707053700582000005707258000
Orion Business Campus
00009707711065701800
Ballycoolin
Dublin 15
Tel.: 01 88 22 222
Fax: 01 88 22 333
Email: sales@ie.vwr.com

Italy

VWR International S.r.l.
Via San Giusto 85
20153 Milano (MI)
Tel.: 02-3320311/02-487791
Fax: 800 152999/02-40090010
Email: info@it.vwr.com

The Netherlands

VWR International B.V.
Postbus 8198
1005 AD Amsterdam
Tel.: 020 4808 400
Fax: 020 4808 480
Email: info@nl.vwr.com

Norway

VWR International AS
Haavard Martinsens vei 30
0978 Oslo
Tel.: 02290
Fax: 815 00 940
Email: info@no.vwr.com

Poland

VWR International Sp. z o.o.
Limbowa 5
80-175 Gdansk
Tel.: 058 32 38 200 do 204
Fax: 058 32 38 205
Email: info@pl.vwr.com

Portugal

VWR International -
Material de Laboratório, Lda
710020007000
Av. Tomás Ribeiro, 43- 3 D
2790-221 Carnaxide
Tel.: 21 3600 770
Fax: 21 3600 798/9
Email: info@pt.vwr.com

Spain

VWR International Eurolab S.L.
7105000000
A-7 Llinars Park
08450 - Llinars del Vallès
Barcelona
Tel.: 902 222 897
Fax: 902 430 657
Email: info@es.vwr.com

Sweden

VWR International AB
Fagerstagatan 18a
163 94 Stockholm
Tel.: 08 621 34 00
Fax: 08 621 34 66
Email: kundservice@se.vwr.com

Switzerland

VWR International GmbH
Lerzenstrasse 16/18
8953 Dietikon
Tel.: 044 745 13 13
Fax: 044 745 13 10
Email: info@ch.vwr.com

Turkey

VWR International Laboratuvar
3700207000000000000
Orta Mah. Cemal Gürsel Caddesi
010702072070070000
34896 Pendik - Istanbul
Tel.: +90216 598 2900
Fax: +90216 598 2907
Email: info@pro-lab.com.tr

UK

VWR International Ltd
Customer Service Centre
Hunter Boulevard - Magna Park
Lutterworth
Leicestershire
4177
Tel.: 0800 22 33 44
Fax: 01455 55 85 86
Email: uksales@uk.vwr.com